


# INDUCTIVELY COUPLED PLASMA EMISSION SPECTROMETER BICP-702

# INDUCTIVELY COUPLED PLASMA EMISSION SPECTROMETER BICP-702

Inductively coupled plasma atomic emission spectroscopy (ICP-AES) is very sensitive technique in emission spectroscopy that measures the mass percentage of the metals in the metal/polymer nanocomposites by exciting its metal atoms/ions by using a plasma and analyzing the emission wavelength of the electromagnetic radiation. Used in Environmental, Metallurgical, Geological, Petrochemical, Pharmaceutical, Food safety.

## BICP-702 INDUCTIVELY COUPLED PLASMA EMISSION SPECTROMETER

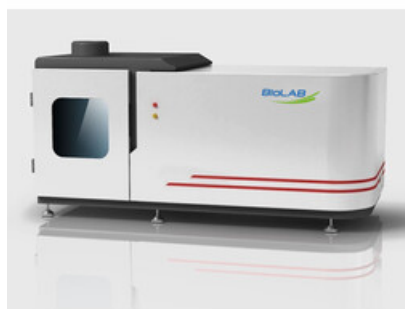

Petrochemical. Ion Beam Etching Holographic Grating, 3600 L/mm or 2400 L/mm.

## SPECIFICATIONS

Model	BICP-702
RF Power technical parameter	
Circuit type:	solid-state RF power supply, with function of automatch
Frequency:	27.12 MHz $\pm$ 0.05%
Frequency Stability	< 0.1 %
Power Output:	800 W - 1200 W
Power Output Stability:	< 0.3 %
Escaped RF radiation:	30 cm away from the instrument, electric field: $E < 2V/m$
Sampling System Technical Parameter	
Output working coil inner diameter:	25 mm
Torque tube:	Three concentric, external diameter 20 mm
Coaxial nebulizer:	Outer diameter 6 mm
Double barrel atomizing chamber:	Outer diameter 34 mm
Gas Flow Controls	
Plasma Argon Flowmeter:	(100-1000) L/h (1.6-16 L/min)
Auxiliary Argon Flowmeter:	(10-100) L/h (0.16-1.66 L/min)
Carrier Argon Flowmeter:	(10-100) L/h (0.16-1.66 L/min)
Pressure Maintaining Valve:	0 - 0.4 MPa
Cooling Water:	Temperature: 20-25 °C, Rate of Flow >5 L/min, Hydraulic Pressure >0.1 Mpa
Spectrometer	
Optics:	Czerny-Turner type
Focal length:	1000 mm

Grating:	Ion Beam Etching Holographic Grating, 3600 L/mm or 2400 L/mm
Reciprocal linear dispersion:	0.26 nm/mm
Resolution:	$\leq 0.007$ nm (3600 line grating); $\leq 0.015$ nm (2400 line grating)
Wavelength range:	3600 line grating: (190 nm ~ 500) nm; 2400 line grating: (190 nm ~ 800) nm
Minimum pace of stepping motor:	$\leq 0.0006$ nm
Exit Slit:	12 $\mu$ m
Entrance Slit:	10 $\mu$ m
Photoelectric Converter Performance	
Photomultiplier tube specification:	R293/R928
Negative HV on PMT:	0 - 1000 V
Stability:	< 0.05 %



**Biolab Scientific Ltd.**

3660 Midland Avenue, Suite 300, Toronto, Ontario M1V 0B8, Canada  
 Email: [contact@biolabscientific.com](mailto:contact@biolabscientific.com) | Website: [www.biolabscientific.com](http://www.biolabscientific.com)