BioLAB

PRODUCT CATALOG




ELISA ANALYZER

CE ISO9001 CERTIFIED

www.biolabscientific.com

ELISA ANALYZER BEM-42001

AUTO ELISA PROCESSOR

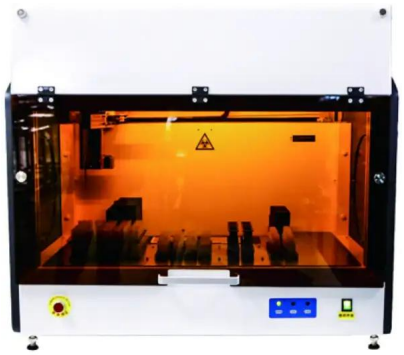

1. 1 robotic arm, 1 pipetting probe(10~1000μl).
2. 2 unit 96 well microplates(independent incubating).
3. 1 unit reader&washer(auto reading and washing).

SPECIFICATIONS

Model	BEM-42001
Sample Unit :	
Sample Racks	Standard 192 sample positions(expandable, up to 384)
Pipetting	10~1000μl
Dispensing System	1 aspirating-dispensing probe(X-Y-Z movement)
Reagent Unit :	
Reagent Racks	Universal reagent position: Standard 6 universal reagent positions(expandable, up to 32);Original reagent bottle: Standard 20 reagent bottles positions(expandable, up to 80)
Pipetting Range	10~1000μl, 1μl stepping
Pipetting Precision	(100μl) CV≤1.0%
Dispensing Time	5 minutes to whole 96 well microplates
Incubation Unit :	
Incubation	2 independent incubators
Temperature Range	RT to 45℃
Temperature Accuracy	±0.5℃
Washing Unit :	
Washing Probes	Two line 8-nozzle manifolds
Wash Containers	2 wash buffers 2L, 1 distilled water, 1 waste water
Washing Residual	≤2μl/well
Reading Unit :	
Reading Channels	8 independent photometric channels, mono and dichromatic reading
Absorbance	0.0~4.0 OD
Spectral Range	400~750nm
Optical Filters	2 standard filters(450, 630nm);2 more on request(405nm/450nm/492nm/630nm)
Data Management :	
Software	Windows 7/10
LIS System	Bi-direction, support HL7 protocol
Results	Absorbance and results reviewable by software
Printer	External optional
Working Conditions :	
Power Supply	AC220V±10%, 50/60Hz; 110V±10%, 60Hz, 400W

Temperature	10~30℃
Humidity	40%~70%
Size&Weight :	
External Size(W*D*H)	935*665*860mm
Net Weight	112kg
Package Size(W*D*H)	1115*920*1398mm
Gross Weight	180kg
Alt Name	Automatic ELISA Analyzer

ELISA ANALYZER BEM-42101

AUTO ELISA PROCESSOR



1. 1 robotic arm, 2 pipetting probes(10~1000μl).
2. 4 units 96 well microplates(independent incubating).
3. 1 unit reader&washer(auto reading and washing).

SPECIFICATIONS

Model	BEM-42101
Sample Unit :	
Sample Racks	Standard 192 sample positions(expandable, up to 552)
Pipetting	10~1000μl
Dispensing System	2 aspirating and dispensing probe(X-Y-Z movement)
Reagent Unit :	
Reagent Position	23 reagent racks, editable
Pipetting Range	10~1000μl, 1μl stepping
Pipetting Precision	(100μl)CV≤1.0%
Washing Unit :	
Dispensing Time	4 minutes to whole 96 to microplates
Washing Probes	Two line 8-nozzle manifolds
Wash Containers	Cleaning fluid(15L), waste water(25L), Buffer 1(5L), Buffer 2(2L),Buffer 3(2L), Buffer 4(2L), with liquid level-sensing, liquid shortage and full alarm
Waste Containers	25L with waste full sensor
Washing Residual	<2μl
Reading Unit :	
Reading Channels	8 independent photometric channels, mono anddichromatic reading
Absorbance	0.0~3.00D
Spectral Range	400~700nm
Optical Filters	2 standard filters(450, 630nm); 2 more on request (405nm/450nm/492nm/630nm)
Reading Accuracy	±1% from 0~1.50D, ±2% from 1.5~3.00D
Incubation Unit :	
Incubators	4 independent units
Temperature Range	RT to 45℃

Temperature Accuracy	±0.5℃
Data Management :	
Software System	Above Windows 7 system
LIS System	Bi-direction, support HL7 protocol
Results	Absorbance and results reviewable by software
Printer	External optional
Working Conditions :	
Power Supply	AC220V±10%, 50/60Hz; 110V±10%, 60Hz, 400W
Temperature	10~30℃
Humidity	30%~80%
Size&Weight :	
External Size(W*D*H)	1235*705*875mm
Net Weight	146kg
Package Size(W*D*H)	1380*860*1415mm
Gross Weight	220kg
Alt Name	Auto ELISA Processor

Biolab Scientific Ltd.
Trillium Executive Center, East Tower, 675 Cochrane Dr, Markham, Ontario L3R 0B8, Canada
Email: info@biolabscientific.com | Website: www.biolabscientific.com