



MEDICAL AUTOCLAVE

BAMN-404

INDEX

1. General Introduction	2
2. Application Scope	2
3. Technical Parameter	3
4. Diagram Specification	4
5. Installation	4
6. Control Panel	5
7. Operation	7
8. Emergency Condition	8
9. Maintenance and Service	9
10. Transportation and Storage	10
11. Accessory	11
Appendix	12

1. General Introduction

This steam sterilizer is a precision instrument specializing in the operation occasion in need of simple, fast and efficient sterilization by the doctor or his/her assistants, and the doctor shall take the responsibility for such work.

This steam sterilizer is equipped with the microprocessor for intelligent control and man-machine interface for convenient operation. With the distinctions in displaying parameter and condition actively, evaluating malfunction automatically, shutting off for self-protection automatically in case of excessive temperature and pressure, this type of steam sterilizer is a reliable product in sterilizing.

2. Application Scope

This product is N-level sterilizer for dental, ophthalmology, operating room, laboratory, small dental equipment, surgical instruments sterilization 121°C/134°C for rapid sterilization of items.

3. Technical Parameter

Chamber size of the Steam Sterilizer (Diameter X Depth) 16L...230mmX360mm

Chamber size of the Steam Sterilizer (Diameter X Depth) 18L...249mmX355mm

Chamber size of the Steam Sterilizer (Diameter X Depth) 23L...249mmX460mm

Rated Voltage.....230V~, 50Hz; 110V~, 60Hz

Sterilizing (Pressure/temp.).....0.9~1.1Bar/121°C

2.0~2.3Bar/134°C

(Both of above are Under Standard Atmospheric pressure)

Rated Power 750VA

Fuse-Melting pipe T15A/T30A

Operating Temp.....0-40°C

4. Diagram Specification

Symbol	Meaning
	CAUTION
	Warning: dangerous voltage
	WEEE MARKING
	DATE OF MANUFACTURE

	SERIAL NUMBER
	CONSULT INSTRUCTIONS FOR USE
	Earthing

Table 1

5. Installation

The clearance between the exterior side surface of the steam sterilizer and the ambient neighboring articles shall be 10cm as retained, and the top surface shall be 20cm retained.

The air-cooling window attached to the exterior surface of the steam sterilizer shall be non-clog by dust or articles, and the steam sterilizer shall be located in the proper air flowing environment by recommendation of the supplier.

The steam sterilizer shall be installed on the horizontal working base.

PREPARATION BEFORE OPERATION

Before operation, please connect well to the power source. Connect the power source hole under the back left side of the steam sterilizer and the power socket by the attached power cable inside the product's package so as to switch on the steam sterilizer. Push down the main power button at the right bottom corner of the front side, when the Switch indicator is bright it means that the steam sterilizer get through with the electric power, and the process then is in initialization status with "LD" being shown on the screen. The steam sterilizer is not heated while under such initialization status.

6. Control Panel

1. Pressure display window

Real-time display the air pressure inside the cavity. Unit: Bar

2. Temperature display window

Real-time display the temperature inside the cavity. Unit: °C

3. Status/ malfunction code number display window

Applied for displaying the status of the steam sterilizer during its working time. See more details in "Appendix working status display form".

When an alarm occurs to the steam sterilizer, the digital pipe of the display will show the alarm code number, the user can find out the malfunction. (Once the malfunction occurring to the steam sterilizer, please contact the service center or distributor immediately).

4. "Temperature" button

It used to be the choice especially for the working temperature. There are two working temperatures for choice: 121 °C or 134 °C, whose light will turn on after being chosen.

5. "UNWRAPPED" button

It's used as the sterilization choice especially for the unwrapped devices. The working temperature is 121°C or 134°C.

After having been chosen, its indicator light is on.

6. "WRAPPED" button

It's used to be the sterilization choice especially for the wrapped devices. The working temperature is 121°C or 134°C.

After having been chosen, its indicator light is on.

7. "START/STOP" button

Press down the starting button for starting the sterilizing process. If you want exit Process, please turn off the electric power.

Note: If forced exit or outage, please wait for 10 minutes, then open the door, In case of the air pressure indoors.

Must wait for the pressure display "0 Bar" can open the door!

8. "READY" indicator light

Door lock indicator light. When the indicator light light, it means can start sterilizing, After launching the indicator light to put out.

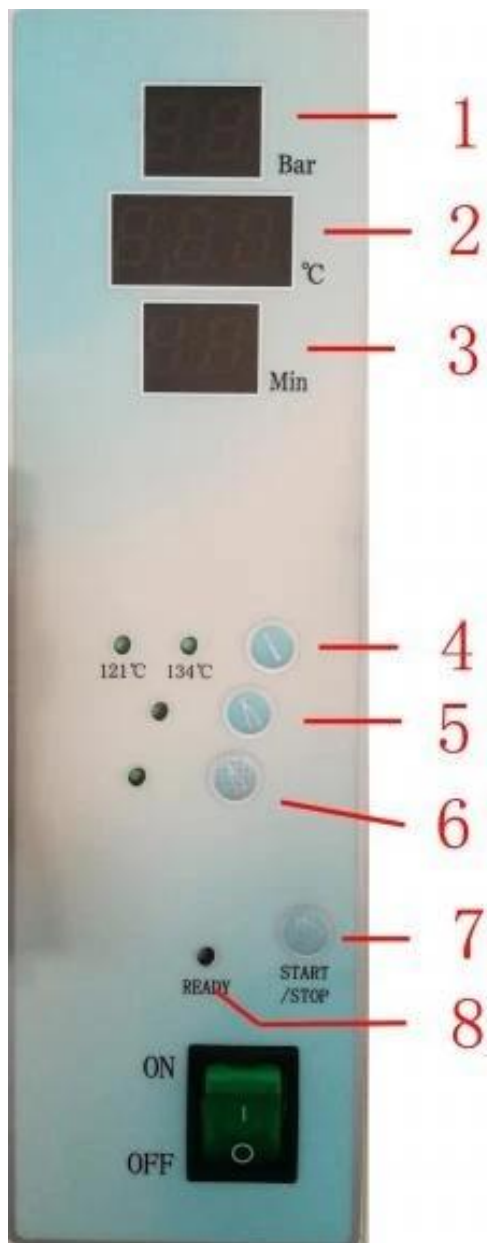


Figure 1

7. Operation

Before operation, please connect well to the power source. when display bright it means that the steam sterilizer get through with the electric power, and the process then is in initialization status with "LD" being shown on the screen. The steam sterilizer is not heated while under such initialization status. Otherwise, you need to close the door completely. Then press the "Start" button to start the sterilizing.

1. Water filling

Please use the measuring cup provided with the sterilizer to pour distilled water directly into the chamber, ensuring that the water level of the distilled water can cover the heating tube and does not exceed the water fender at the door of the sterilization chamber.



Make sure there is enough water in the chamber before each time working!

2. Connect the drain pipe and put one end into a container, put the apparatus to be sterilized onto the mesh trays which are inside the chamber, then close the door and make sure to revolve the door handle to the maximum position.

3. Lock indicator "READY" light,press the "START" key to start working.

Note: If the door is not completely closed, the machine can't work when you press down the "START" button. If the door is opening during the working process, the working status display will flash "E5"as an alarm and the steam sterilizer will stop working until restart again by switching off the power and dismissing the alarm.

4. Status displays "ED" and has a beep after the sterilizing process, then you can open the door and take the sterilized apparatus out. Must wait for the pressure display "0 Bar" can open the door!

5. Please shut off the main power supply when you don't use the steam sterilizer. (The light of power is off).

6. Sterilizing cycle

PROCEDURE	TEMPERTURE	PRESSURE	TIME
UNWRAPPED	134°C	2.1Bar	4 minutes
	121°C	1.1 Bar	10 minutes
WRAPPED	134°C	2.1 Bar	8 minutes
	121°C	1.1 Bar	20 minutes

Table 2

8. Emergency Condition

During the running time, the steam sterilizer will automatically raise the alarm, release pressure, stop heating and display the warning code. (The definition of the warning code is as the below: malfunction code and resolving method) for ensuring the safety of the operator if the emergencies occur.

Any emergencies happen, please check the warning code table for resolving the according malfunctions. If not possible to resolve, please contact the dealers. We will try our best to provide help to you in a short time.



Must wait for the pressure display "0 Bar" can open the door,



There will be set aside heat and residual hot water, Operators also need to keep away from it , to prevent burns!

Malfunction code and resolving measures.

0	E	Heating failure	Check the heating heater Check vent valve of water is normal Check water level Check for gas leaking away
		Failure to maintain the temperature	Check temperature
0	E		sensor
			Check vent valve of
			water is normal
			Check water level
0	E	Excessive Temperature (temperature sensor fault)	Check temperature sensor
0	E	Pressure can not be released	Check the exhaust, drain valve
0	E	Door switch bounce	Check the door knob, microswitch

Table 3

Others:

1. Turn on the power, display board doesn't show. Check if the display board loosen or not.
2. When or after closing the door, Lock indicator not light, check if the feeler lever of micro switch touches the micro switch well.

9. Maintenance and Service

1. Disinfect and clean the interior surface of the steam sterilizer room by Medicinal alcohol once a month.
2. Replace the fuse-melter.

(1) Shut off the power

(2) Revolve the fuse base by counter-clockwise by screwdriver to bring out the melting fuse to be replaced;

(3) Replace the new fuse and reset the fuse base on the original position, then use the screwdriver to fasten the base by clockwise.

(4) Check the correctness of the parameter of the new fuse replaced.

3. Clean the sealing ring periodically

The user shall clean the sealing ring periodically for avoiding the influence to the seal caused by the dust/dirt left due to the long period of use. Use the smooth cloth with distilled water to wipe the surface of the sealing ring or sealing cap gently.

The user shall discharge the sealing ring for further cleaning or replacement if the air-leaking problem can not be resolved after the above process (The user shall discharge the sealing ring periodically for cleaning and inspection as recommendation by the supplier). Put back the ring to the original door groove after cleaning. Most Important: the inset work must be done equably to the groove During the installation, the laid four equal points of the ring must be inserted to the groove firstly, later for the same work for the remaining segments of the ring. After finishing, press the sealing ring equally by the force of hand.

4. Shut off the power before service or components' replacement, and the service or replacement work shall be done by the supplier or his designated technician.

10. Transportation and Storage

The steam sterilizer shall be transferred and stored with the below conditions: Ambiance temperature: -40°C --+55°C

Relative humidity: < 85%

Atmospheric pressure: 500HPA-1060HPA

11. Accessory

1.	Draining pipe	1 pc
2.	Tray	3 pcs
3.	Plug	1 pc
4.	Bracket	1 pc
5.	Manual holder	1 pc
6.	Fuse	2 pcs

7.	Operation manual	1 pc
8.	Measuring cup	1 pc
9.	Sealing ring	1 pc
10.	O ring of tap	2 pcs

Table 4

Appendix

I Working status display table

NO .	Display	Explain
1	Ld	Prepare/preheating state
2	He	Heating state
3	working time	Sterilization state
4	Ed	end-of-job

Table 5

II Steam Way:steam ff Map

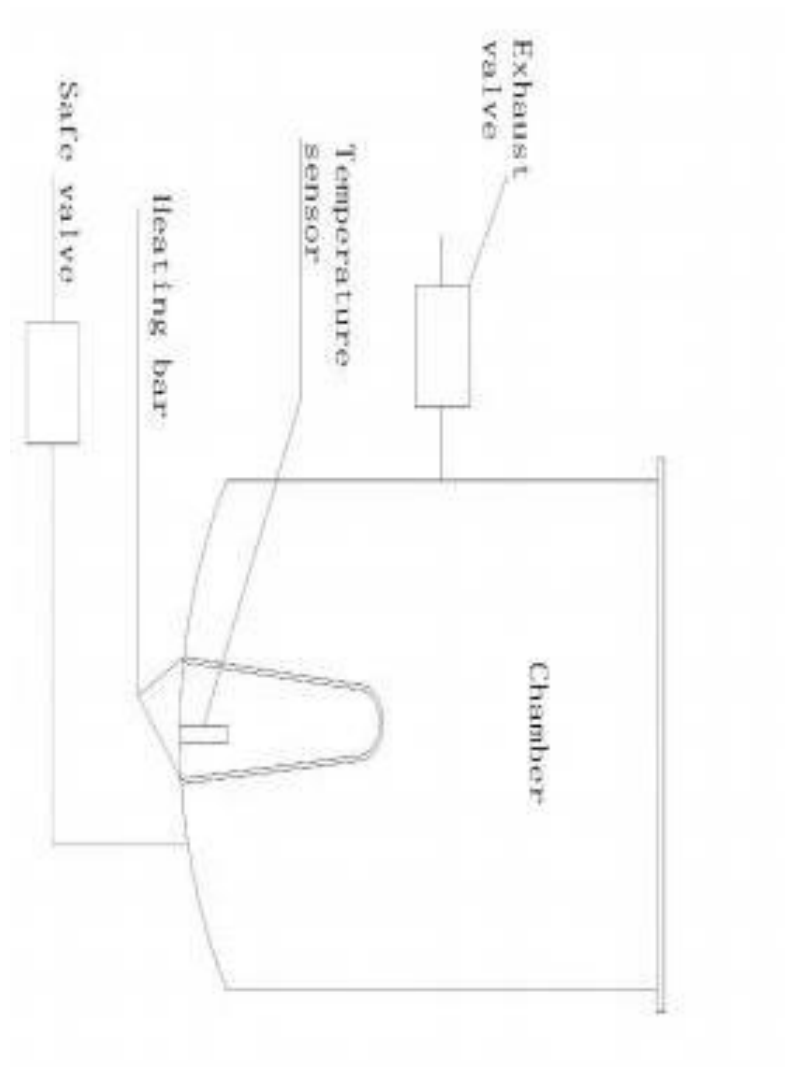


Figure 2

III Wiring Map

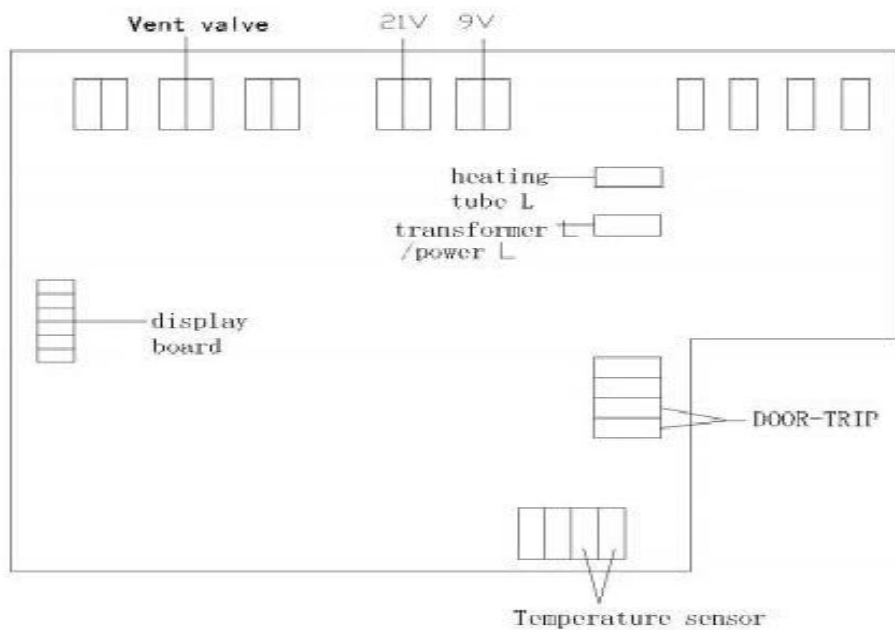


Figure 3



Biolab Scientific Ltd.

Trillium Executive Center, East Tower, 675 Cochrane Dr, Markham, Ontario L3R 0B8, Canada
Email: info@biolabscientific.com | Website: www.biolabscientific.com