

Operation Manual



BBBF-201

Blood Bank Refrigerator

Thank you for Choosing Biolab products. Please read the "Operating Instructions" and "Warranty" before operating this unit to assure proper operation.

Index

1. Installation and operation	04
2. Standard Control System	07
3. Product description	11
4. Cleaning	13
5. Maintenance	14
6. Disposal	16



CAUTION!

All internal adjustments and maintenance must be performed by qualified service personnel.

This appliance can be used by children aged from 8 years and above and persons with reduced physical, sensory or mental capabilities or lack of experience and knowledge if they have been given supervision or instruction concerning use of the appliance in a safe way and understand the hazards involved.

Children shall not play with the appliance.

Cleaning and user maintenance shall not be made by children without supervision.



Environmental Protection

Discarded electric appliances are recyclable and should not be discarded in the domestic waste! Please actively support us in conserving resources and protecting the environment by returning this appliance to the collection centers(if available).



Important operating and/or maintenance instructions. Read the accompanying text carefully.



Potential electrical hazards. Only qualified persons should perform pr°Cedures

associated with this symbol.



Hot surface(s) present which may cause burns to unprotected skin or to materials which may be damaged by elevate temperatures.



Extreme temperature hazards, hot or cold.

Use special handling equipment or wear special, protective clothing.

01 Installation and operation

Safety Information

All electrical work must be executed by suitably qualified persons. When using any electrical appliance, safety precautions must always be observed.

Do not use this appliance for other than its intended use. This product is intended for use as a Blood Bank Refrigerator. Consult your supplier for alternatives.

Do not cover the front grille or block the rear air entry by placing object up against the cabinet.

Please close attention, when used by or near children, infirm persons.

Ensure adequate ventilation.

Do not probe any openings.

Do not touch any moving parts or hot surfaces.

Regulations require that all electrical work be carried out by authorized persons. For your own safety and that of others please ensure this is done.

Do not overload the power supply. Always ensure on the rating label. The rating label is located.

If have any problem, please consult a qualified electrician. Caution: Never use extension leads or multiple adaptors.

If the mains supply cord is damaged, it must be replaced by the manufacturer, its service agent or similarly qualified and skilled persons in order to avoid hazard.

Disconnect the mains power supply before attempting any cleaning, removal of any covers, or maintenance work.

Do not store explosive substances, such as aerosol cans with flammable propellant.

Warning: Do not use mechanical devices or other means to accelerate the defrosting process. Defrosting is performed automatically.

Warning: Do not damage the refrigeration circuit.

Warning: Do not use electrical appliances inside the storage compartment of this appliance.

1.2 Assembly

Remove the appliance from the packaging and peel off any protective film from all surfaces.

Fit the shelf support clips onto the shelf support strips, making sure that the clips for each shelf are of the same height and that they are securely engaged on the support strip.

Unwrapping each shelf carefully, to prevent damaging their protective coating or surface finish.

Position the shelves onto the clips.



Please dispose of all waste packaging appropriately and in accordance with all I°Cal recycling laws.



warning Do not overload the power supply. Always ensure that the power supply is adequate for the electrical requirements specified on the rating label and never use extension leads or multiple adaptors.

Positioning the Blood Bank Refrigerator

- Please position the cabinet carefully being careful not to bump it.
- The power supply flex exits the Blood Bank Refrigerator at the bottom right hand side (as viewed from the front). For ease of access; the flex should be retrieved prior to positioning the Blood Bank Refrigerator in its final location.
- The maximum recommended ambient temperature for this Blood Bank Refrigerator is 38°C
- Avoid positioning the appliance in direct sunlight or damp areas.
- Allow adequate space for the door(s) to fully open.
- Ensure that this Blood Bank Refrigerator is positioned on a level surface, so as to allow the door(s) to shut and seal correctly, as well as to allow proper drainage from the evaporator tray, to prevent any overflow. If necessary, adjust the screw feet of the appliance to make it level.

Note: If the unit has not been stored or moved in an upright position, let it stand upright for approximately 12 hours before operation.

Ventilation

- All models must have clear and unobstructed ventilation from the entire surface area of the front grille.
- The 2 and 3 door models may be built into an enclosure without the need for ventilation other than at the front.
- The single door of Blood Bank Refrigerators must have a minimum ventilation space of 20mm at sides and rear.
- Dimensions of the space to be provided for the appliance are referenced on page 13 of this manual.
- Dimensions and position of the means for supporting and fixing the appliance within this space are referenced on page 13 of this manual.
- WARNING: Failure to provide the minimum ventilation space will harm the performance of your Blood Bank Refrigerator could cause fire and will invalidate the warranty.
 - MARNING: Keep clear of obstruction all ventilation openings in the appliance enclosure or in the structure for building in.

Power Supply

The Blood Bank Refrigerator uses a three-pin plug which must be well grounded. Never ground the Blood Bank Refrigerator through a gas pipe, tap water pipe OR the grounded wire of single-phase power supply etc. Never share same circuit with other appliances. Before plugging in your Blood Bank Refrigerator for the first time make sure the power cable is free from damage and check that your voltage corresponds to that on the serial plate.

Once plugged in the display will show the temperature inside the Blood Bank Refrigerator and the compressor will run late on (the indicator light of cooling will be on at the same time). This temperature is the actual temperature recorded by the probes inside the Blood Bank Refrigerator and as the fridge cools to the set point (factory set at 4°C/39°F) so the number on the display will descend accordingly. If power is cut off, wait for at least 5 minutes before plugging the unit in again to avoid damaging the compressor.

02 Standard Control System

Plastic Panel

Touch Screen Display



USB Interface

Control Panel



4.3"LCD touch screen, Main interface



4.3"LCD touch screen, Setting Options



4.3"LCD touch screen, Temp set



7"LCD touch screen, Password set (Initial password 1000)



4.3"LCD touch screen, Information view

2.2 FUNCTIONING STANDARD CONTROL

Introduction

The refrigerator/freezer is equipped with a latest generation Electronic Controller, with a LCD alphanumeric display, to display temperature and working operations with an accuracy of 0.1°C. The controller gives maximum safety in case of alarms and fault conditions, signaling critical conditions and recording every event in order to help the service engineer to speed up the analysis and thus the fixing of any problems. Safety is at the highest level with alarms for High and Low temperature, power-failure, door open as well as auto-test. What is more, the STANDARD Control is equipped with an internal cl°Ck to catalog all the events.

2.2.1 SWITCHING ON*

*After positioning the equipment, stand for it at least 12 hours, then connecting the power cord of the equipment, and turn on the switch of backup battery.

2.2.2 SWITCHING OFF*

Turn power off.

2.2.3 Temperature Settings

The Refrigerator temperature set point ranges from $+1^{\circ}$ C to $+15^{\circ}$ C. The default factory temperature set point is $+4^{\circ}$ C.

To change temperature settings, you need to access SETTINGS menu. All menu options under SETTINGS menu are used to configure the settings for temperature chamber only.

Note: If the set point is changed, the high and low alarm limit will change automatically. For example: initial temperature set point: 4°C; low alarm limit: 1°C; high alarm limit: 9°C. If the temperature set point is subsequently changed to5°C, then the high and low alarm limit will adjust automatically to 10°C and 2°C.

2.3 Operating the Freezer

2.3.1 Product Loading

Loading of warm product into the freezer should be done in batches. Do not fill the freezer with product of more than 20 percent of the volume at one time as this pr°Cess might introduce too much heat load into the freezer. Allow freezer to stabilize. Once the temperature of the freezer returns to the set point, another batch of product can be loaded in.

Fill an upright freezer by starting at the bottom near the temperature probe and add products to shelves, one shelf at a time. Allow freezer to recover to set point or temperature between shelves.

Fill empty shelves with pre-cooled samples to help reducing the temperature rise during loading.

At any time, to ensure not more than 10 kg product be loaded in at one time.

Blood Bank Refrigerator BBBF-201

Always make sure the vacuum relief port is free of frost and ice, to allow for timely re-opening of the main door.

The Refrigerator/Freezer are designed for long term storage. It is recommended that only pre-frozen products be placed in the unit as it will reduce the amount of heat load that must be absorbed by the freezer at one time.

2.3.2 Opening and Closing Doors

Main door and inners doors should be closed tightly at all times. When taking the samples out, open the main door and then open only one inner door at a time. "DOOR OPEN" message will be displayed as soon as the main door is open. If the main door is left open for more than the pre-determined time (MAIN MENU > ADMIN > DOOR ALARM TIME), the audible alarm will ring to remind user to close the door.

2.3.3 Locking the Main Door

Main door can be locked with the standard key set provided.

2.4Alarm

2.4.1 High/Low Temperature

This alarm is activated when the actual temperature inside the chamber has reached the temperature set point and for some reason exceeds high/low alarm temperature set point. The message "HIGH ALARM" or "LOW ALARM" will be displayed on the 4th row of the LCD. The High/Low Temp LED indicator will light and an audible alarm will ring. The audible alarm can be muted by pressing the MUTE key.

2.4.2 Hot Condenser

This alarm is activated when the sensed temperature at condenser outlet is 15°C higher than the sensed ambient temperature displayed on LCD. The message "HOT CONDENSER" will be shown on the 4th row of the LCD. No audible alarm will ring but the Hot Condenser LED indicator will light. This alarm will not stop the freezer operation.

2.4.3 Low Battery

This alarm is activated whenever the battery voltage is lower than 11.5 VDC or the battery switch behind the right bottom door is turned off or the battery is not properly installed. "LOW BATTERY" message will appear on the 4th row of the main display of the LCD. Low Battery LED indicator will light. Audible alarm will ring. The audible alarm can be muted by pressing the MUTE key.

2.4.4 Other Alarms

All of the below alarms will cause Other Alarms LED indicator to light.

2.4.4.1 Power Failure

This alarm is activated whenever there is a power failure and the Refrigerator/Freezer control system is still running on battery power. "POWER FAILURE" message will appear on the 4th row of the LCD. Audible alarm will ring. The audible alarm can be muted by pressing the MUTE key.

2.4.4.2 Sensor Failure

This alarm is activated when the sensor for chamber temperature (CHAMBER) is defective or not properly connected. The compressor will not start to cool down the chamber. "XX SENSOR FAILURE" message will appear on the 4th row of the LCD. Audible alarm will ring. The audible alarm can be muted by pressing the MUTE key.

2.4.4.3 Door Open


"DOOR OPEN" message will appear on the 4th row of the LCD as soon as the main door is opened. Audible alarm will ring after pre-determined time set in the menu DOOR ALARM TIME under ADMIN menu. The audible alarm can be muted by pressing the MUTE key.

2.4.4.4 High Ambient

"HIGH AMBIENT" message will appear on the 4th row of the LCD as soon as the ambient temperature displayed on the LCD is above 32°C. Audible alarm will ring immediately. The audible alarm cannot be muted. This alarm will not stop the freezer operation.

03 Product Description

3.1Product parts name

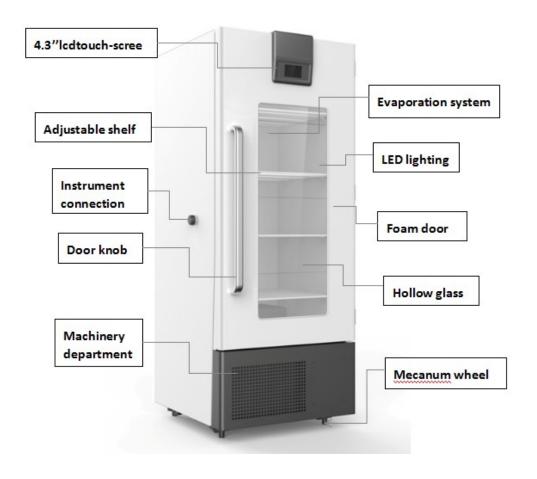

3.2 Product model specification

	Model	BBBF- 201	BBBF- 202	BBBF-203	
Technic al Data	Cabinet type	Vertical	Vertical	Vertical	
	ClimateClass	N	N	N	
	CoolingType	Forced air cooling	Forced air cooling	Forced air cooling	
	DefrostMode	Auto	Auto	Auto	
	Refrigerant	R134a/ R600a	R134a/ R600a	R134a/R600a	
Perform ance	Temperature Range (°C)	4±2	4±2	4±2	
Control	Temperature Control	Micropr°Cessor Control Board			
	Display	LCD			
Material	Interior	Galvanized steel powder coating			
	Exterior	Galvanized steel powder coating			

Electric al Data	Voltage/ Frequency	220V/50Hz &110V/60Hz		
	Capacity (L)	328	420	535
Dimensi ons	External Dimension (<i>W/D/H</i>)	640*690* 1860 (mm)	640*820*1 860 (mm)	780*820*1860 (mm)
	Shelf	5	5	5
Accesso	Test Hole	Y	Y	Υ
ries	Chart Temperature Recorder	Optional	Optional	Optional

04 Cleaning

- MARNING: You must disconnect the plug before cleaning or maintenance.
- Do not use abrasive cleaning agents which may scratch and harm the delicate interior finishes of your appliance.
- Always wipe dry after cleaning.
- An agent or qualified technician must carry out repair if required.

4.1Clean the filter of single door Blood Bank Refrigerator

- The filter must be kept clean and free of dust at all times. It is recommended that the cleaning routine be conducted at interval appropriate to the speed of accretion of dust on the filter and in any event at least every month. Failure to keep the filter clean will damage the refrigeration system and invalidate the warranty.
- Pull the filter upwards to remove it from its locating place under the glass door.
- Use a vacuum cleaner, preferably with a rush attachment, to remove built up dust.
- Refit the filter to its original location to ensure continual efficient operation is maintained.

4.2Clean the condenser

 The condenser must be kept clean and free of dust at all times. It is recommended that the cleaning routine be conducted at interval appropriate

Blood Bank Refrigerator BBBF-201 -

to the speed of accretion of dust on the condenser. Failure to keep the condenser clean will damage the refrigeration system and invalidate the warranty.

• MARNING: The condenser is a delicate component and is easily damaged. Never use a stiff brush or sharp objects to clean it. Never use water.

05 Maintenance

If your appliance develops a fault, please check the following table before making a call to the helpline.

Fault	Possible Cause	Action
The appliance is not working	The unit is plugged in correctly	Check the unit is plugged in correctly
	Plug or lead is damaged	Call Our agent or qualified technician
	Power supply	Check power supply
	Internal wiring fault	Call Our agent or qualified technician
The appliance turns on, but the temperature is too high or too low	Filter or condenser blocked with dust	Clean filter or condenser
	Doors are not shut properly	Check doors are shut and seal are not damaged
	Appliance is located near a heat source or air flow to the condenser is being interrupted	Move the appliance to a more suitable location
	Ambient temperature is too high	Increase ventilation or move appliance to a Blood Bank Refrigerator position
	Insufficient airflow to the fans	Remove any blockages to the fans
	Appliance is overloaded	Reduce the amount stored in the appliance
	Factory default parameters adjusted	Call Our agent or qualified technician
The LED lights not working	Led light short Leaded damage	Call Our agent or qualified technician
The appliance appear BT alarm	See description below	See description below
The appliance is unusually loud	The appliance is touching a neighboring object	Check installation position and change if necessary
	The appliance has not been installed in a level or stable position	Check installation position and change if necessary

06 Disposal

If in any doubt, please consult your Local Authority, contact us or contact the reseller from whom you purchased the appliance.



BIOLAB SCIENTIFIC LTD.

3660 Midland Avenue, Suite 300, Toronto, Ontario M1V 0B8 Canada Email: contact@biolabscientific.com Tel: +1 707 533 1445 Website: www.biolabscientific.com