



ORBITAL SHAKER

BSOT-205

INDEX

1. Safety Warnings and Guidelines	2
1.1 Important operation information of the security	2
1.2 Security	3
1.3 Instruments Maintenance	4
1.4 After Service	4
2. Introduction	5
3. Specifications	6
4. Preparation	7
5. Operation Guide	9
5.1 Start/Stop	9
5.2 Speed setting	10
6. Failure Analysis and Trouble Shooting	10

1. Safety Warnings and Guidelines

1.1 Important operation information of the security

Users should have an entire conception of how to use the instrument properly before operating it. Please read this operation manual carefully before using the instrument.



It is forbidden operating before read the operation manual. Read the guidelines and directions below and carry out the countermeasure according to them.

1.2 Security

The operation, maintenance and repair of the Instrument should comply with the basic guidelines and the remarked warning below. Otherwise, it will affect the scheduled using life of the Instrument and the protection provided.



This product is a normal and an indoor Instrument which conforms to Standard B style- I type- GB9706.1.



Before operation, read the manual carefully. These units are designed for using in the laboratory environments by who're knowledgeable in safe laboratory practices.



The operator should not open or repair the instrument by himself. Otherwise, the instrument will lose the qualification of repair guarantee or cause accidents. The company will repair the instrument based on warranty description.



Before connecting the power supply, make sure that the voltage of the power supply is consistent with the voltage required by the instrument. And ensure that the rated load of the power socket is not less than the requirements of the instrument.

If the power cord is damaged, it must be replaced. Replace with a power cord of the same type and specification. Do not press anything on the power cord when this instrument is in use. Do not place the power cord where people are walking.

Be sure to hold the plug when pulling out the power cord. Make sure that the plug is fully plugged into the socket and do not pull the power cord when pulling out the plug.



The instrument should be put in the place where of low humidity, little dust, no water, no sunshine or hard light, and of good aeration, no corrosively gas or strong disturbing magnetic field, and far away from central heating, camp stove and other hot resource. Do not put the instrument in wet and dusty place. The vent on the instrument is designed for aeration. Do not wall up or



Power off when operation finished. If do not use the instrument for a long period, pull off the connector plug, cover a piece of cloth on the instrument to prevent from dust.



Pull the connector plug from the jack at once in the following case, and contact the vendor.

- There is some liquid flowing into the instrument;
- Drenched or fire burned;

- Abnormal operation: such as abnormal sound or smell;
- Instrument dropping or outer shell damaged;
- The function has obviously changed.

1.3 Instruments Maintenance

The instrument and the accessories should be cleaned by cloth drenched with alcohol.

If the surface of the instrument is smudged, it can be cleaned with a soft cloth dampened with a cleaning paste.

1.4 After Service

1. Warranty Description

Within one month of delivery, the company is responsible of exchange for breakdown caused by material or manufacture. Within 12 months of delivery, the company is responsible of free repair for breakdown caused by material or manufacture. Proven with defect under warranty, the company will exchange the instrument or free repair it alternatively. Instrument under warranty period should be delivered to the appointed maintenance department by user. Freight from user to maintenance department will be borne by user. Freight for instrument resent to user will be borne by the company. Repair out of warranty will be charged reasonable cost.

2. Warranty Coverage

Breakdown due to improper use, operation in inappropriate conditions, maintain or refitting without authorization are not in warranty coverage.

2. Introduction

Decolorization shaker is widely used in Coomassie blue dyeing and swaying during decolorization, fixation of electrophoresis gel, fixation, dyeing and saliency in silver nitrate dyeing. Development and fixation of X-ray film in autoradiography experiments. After electrophoretic transfer, further process of cellulose membrane. Such as molecular hybridization, antigen-antibody reaction and staining, and can be used for cell culture and cell membrane transfer.

Features:

1. Compact appearance, space saving, powerful function and strong compatibility.
2. Suction cup type machine feet, super shockproof, high speed and smooth, no noise.
3. large platform design, placing more samples, strong load capacity.
4. Three models are available, the configuration performance is from low to high, to meet more choices.

3. Specifications

1. The Normal Operation Condition

Ambient Temperature: 4C

45°C Relative Humidity: ≤70%

Power: AC110 / 220V, 50/60Hz

2. The Basic Parameters and Specifications

Type	BSOT-205
Speed Range	0~300rpm
Time Range	/
Digital Display	/
Radius of gyration	10mm
Max Load Capacity	2.5Kgs
Motor Parameters	DC motor stepless speed regulation
Platform Size	330mmx430mm
Voltage	AC110 / 220V,50/60Hz
Power	25W
Fuse	250V,1A,φ5x20
Dimension	330mmx490mmx145mm
Net Weight	9.5Kgs

Table 1

4. Preparation

It mainly describes the instrument's mechanical structure, the keyboard and functions of each key, as well as preparations before power on. Please learn this chapter well before the orbital shaker is to be operated at the first time.

1. Structure Description



Figure 1




Figure 2

2. Keyboard and Display Panel



Figure 3

3. Key Function



Turn the knob to the right to increase the speed. Rotation to the left is the opposite.

4. Power Connection

Place the instrument on a stable, horizontal work table. Insert the cylindrical socket of the power cord into the power input socket at the back of the instrument as shown. Connect the other end of the power cord to the power grid. The grid voltage is required to be 110V or 220V.



Figure 4

5. Platform Installation

The decolorization shaker series can be equipped with four type of platforms




Platform



Conical Flask Stand
250ml can put 12pcs



Conical Flash Stand
100ml Can put 20 pcs

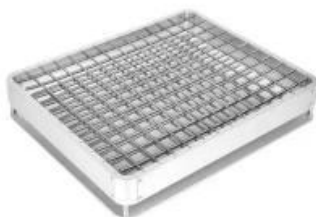

Universal Platform

Figure 5

Platform installation steps:



Figure 6

5. Operation Guide

5.1 Start/Stop

1. Turn on the power switch to start running the instrument. Turn the adjustment knob to the right to run the instrument.
2. Turn the adjustment knob to the right to run the instrument.

5.2 Speed setting

1. Turn the adjustment knob to the right to increase the speed
 2. Turn the adjustment knob to the left to decrease the speed.
- It is recommended to increase the speed slowly to ensure that the container is stable and prevents spillage.

6. Failure Analysis and Trouble Shooting

Failure Analysis and Processing Procedures

No.	Phenomenon	Possible Causes	Processing Procedure
1	No signal display when power on.	No power	Check the power
		Broken switch	Exchange the switch
		Others	Contact with the seller
2	Shaking heavily	Samples placed imbalanced	Place the samples evenly
3	Actual speed and displayed speed are not matching	Broken controller	Contact with the seller
4	Err displays	Speed out of control	Contact with the seller
5	Knob does not work	Broken button	Contact with the seller

Table 2

Appendix A:Wiring Diagram of Decolorization shaker
(Below diagram is just for reference. It is subject to change without prior notice.)

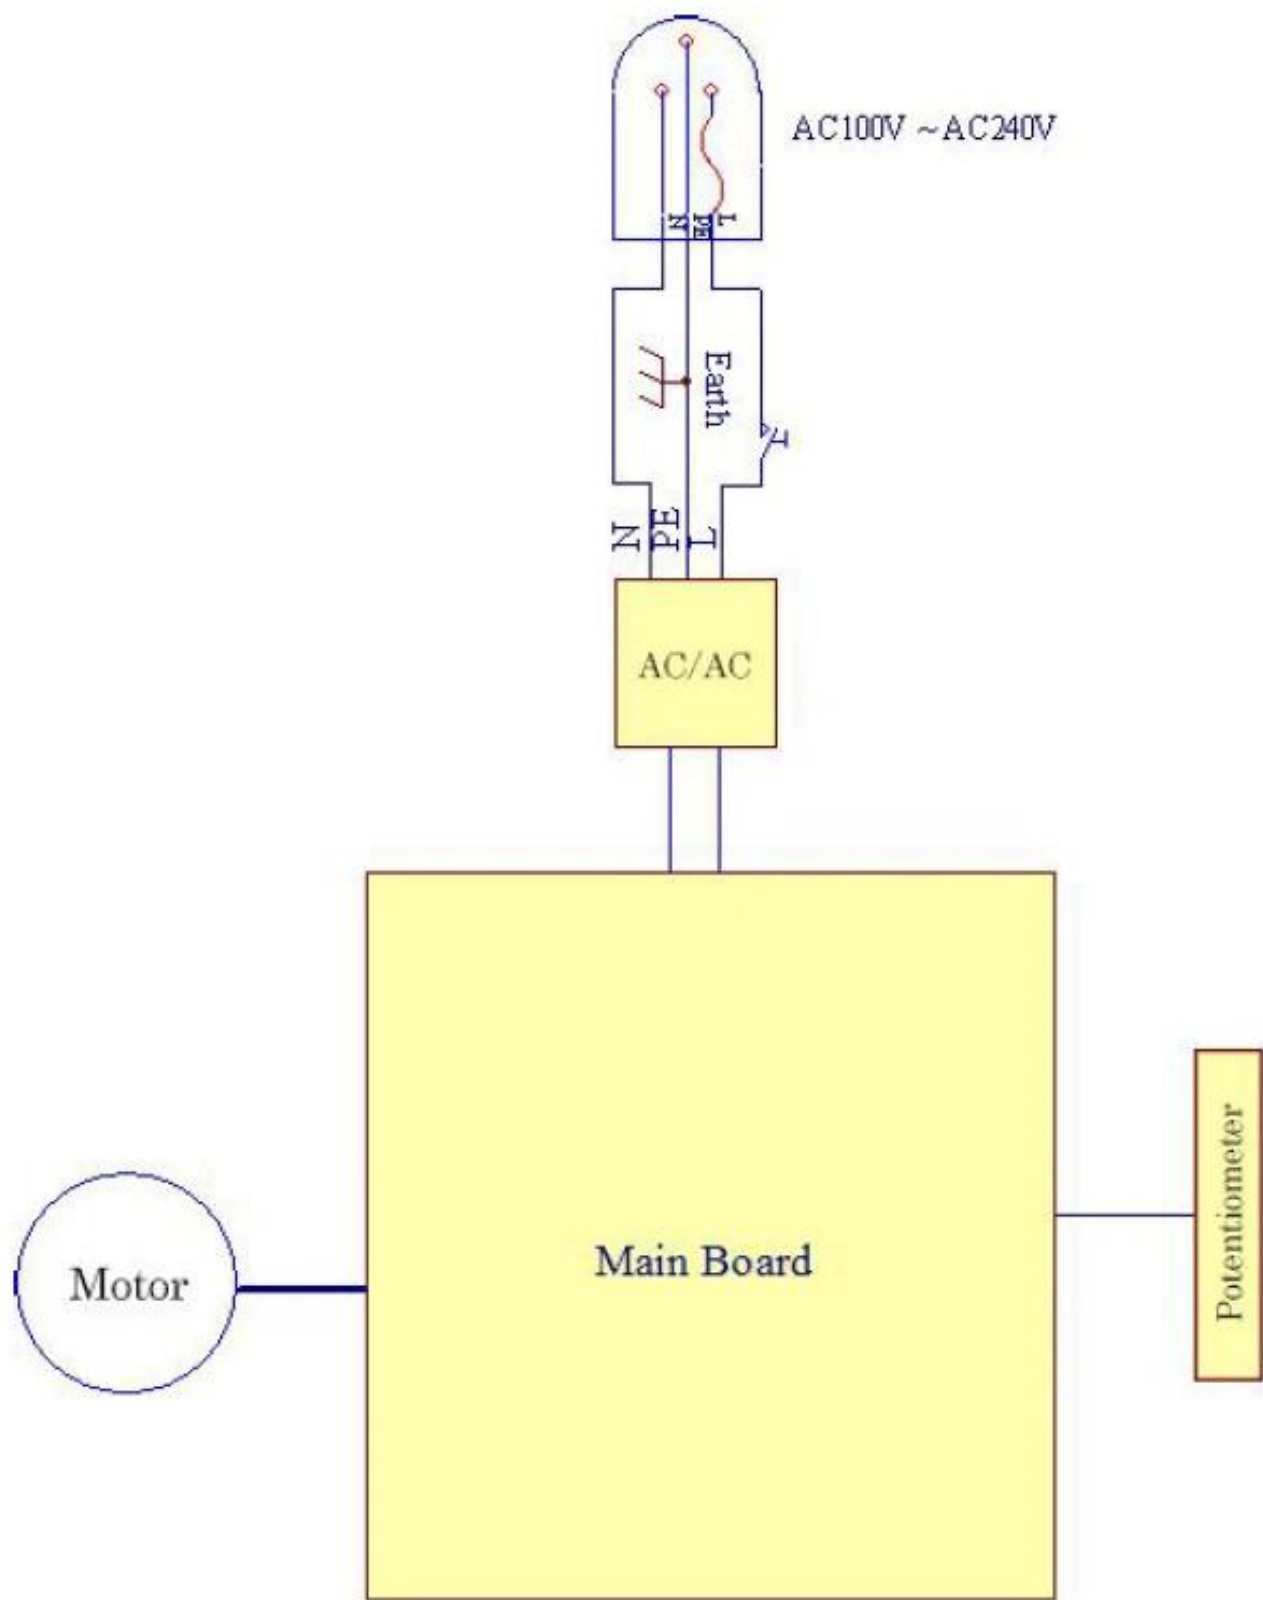


Figure 7



Biolab Scientific Ltd.

Trillium Executive Center, East Tower, 675 Cochrane Dr, Markham, Ontario L3R 0B8, Canada
Email: info@biolabscientific.com | Website: www.biolabscientific.com