



POUR POINT TESTER

BPTL-221

INDEX

I. Product overview	2
II. Method Summary	2
III. Apparatus and materials	3
IV. Preparation	6
V. Operation Steps	7
VII. Common faults and troubleshooting	12
VIII. Quality Assurance	13

I. Product overview

This instrument is mainly suitable for determine the pour point and cold filter plugging point of petroleum products.

1. Applicable standards: GB/T3535, SH/T0248
2. Temperature control method: Imported PID digital display temperature controller, digital display temperature (continuously displayed during testing), with an accuracy of 0.1 °C.
3. Temperature control accuracy: -60 ± 0.1 °C -40 ± 0.1 °C
4. Operating environment temperature: ≤ 25 °C
5. Refrigeration method: metal bath refrigeration, enclosed compressor refrigeration, environmentally friendly refrigerant, fast refrigeration speed.
6. Work unit: two troughs and four holes
7. Integrated structure, easy to move.
8. The instrument is made of cold-rolled steel plate and has a surface treated with electrostatic spraying, which is corrosion-resistant and easy to clean.
9. The instrument welding adopts butt welding technology, without solder joints, with a beautiful and elegant appearance.


II. Method Summary

The operating principle of pour point is: after pre heating, the sample is cooled at a specified rate, and the fluidity of the sample is checked every 3 °C. Record the lowest temperature at which the sample can flow as the pour point.

The operating principle of the cold filter point is to cool the sample under specified conditions and use a controllable vacuum device of 2KPa to allow the sample to pass through a standard filter and be sucked into a pipette. Repeat this step for every 1 °C lower than the previous temperature of the sample until the amount of wax like crystal precipitation in the sample is sufficient to stop the flow or reduce the flow rate. Record the temperature when the pipette is full of sample for more than 60 seconds or cannot fully return to the test cup as the cold filter point of the sample.

III. Apparatus and materials

Pour Point

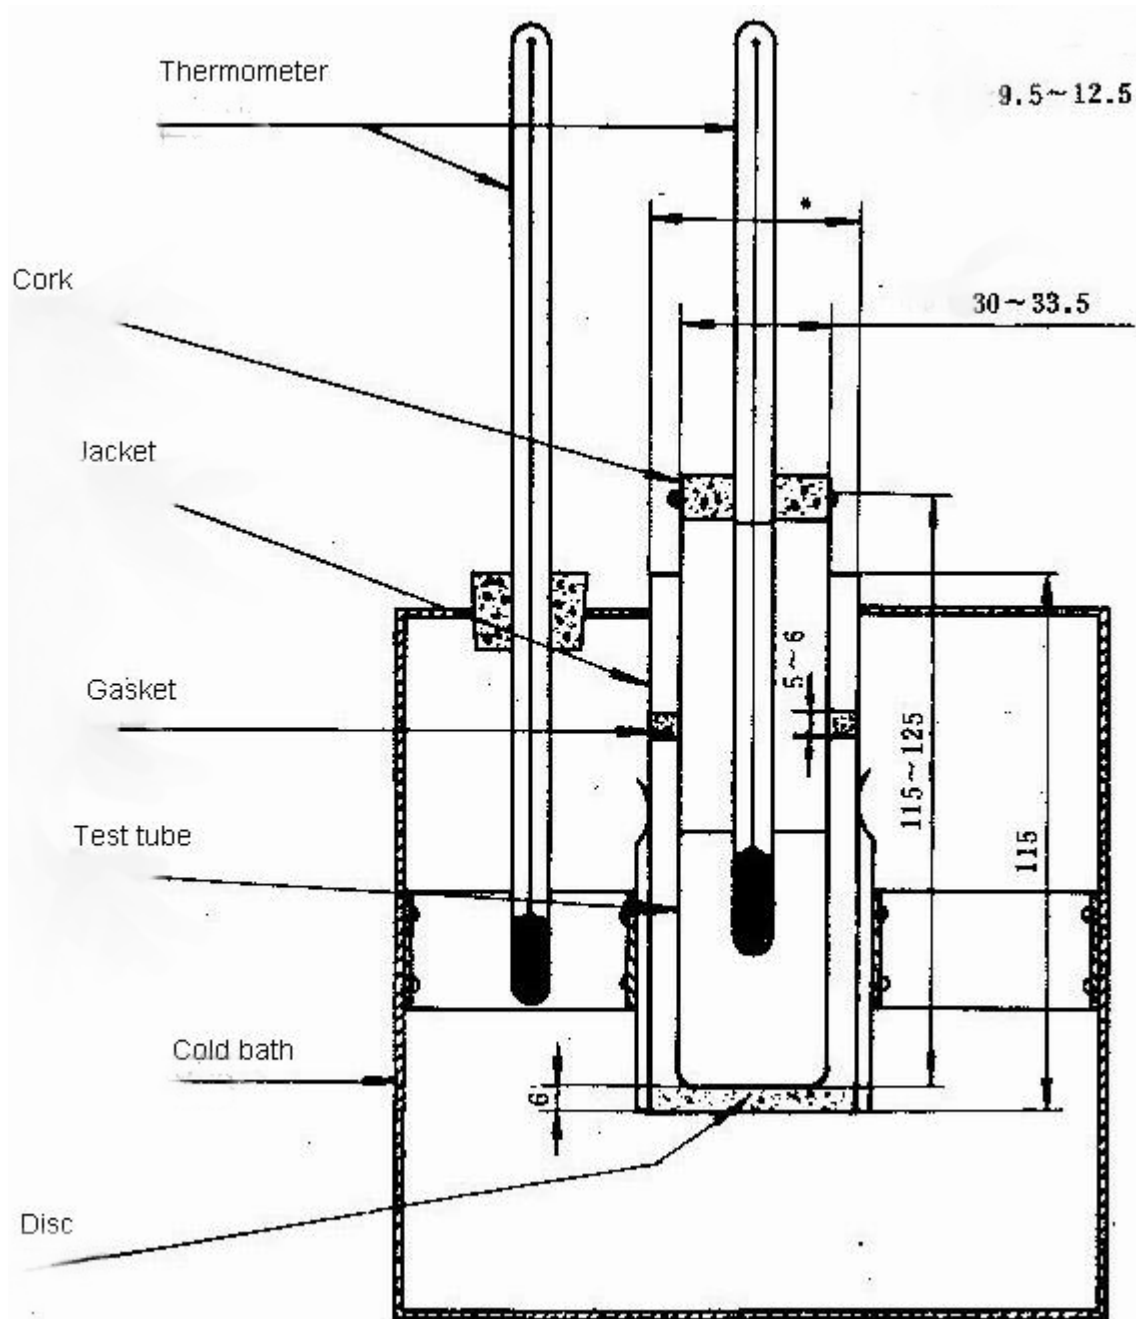

1. Test tube: A cylindrical shape made of transparent glass with a flat bottom. The inner diameter of the test tube is 30.0-32.4 millimeters, and the height is 115-125 millimeters. A long scribed line is marked 54 ± 3 millimeters from the bottom of the test tube, indicating the height of the liquid level inside.

2. Thermometer:

2.1 High cloud point and high pour point thermometers: temperature measurement range $-38 \sim 50$ °C, with a division value of 1 °C

2.2 Low cloud point and low pour point thermometers: temperature measurement range $-80 \sim 20$ °C, with a division value of 1 °C

3. Cork plug: used with a test tube, with a hole for inserting a thermometer punched in the center of the plug.

4. Sleeve: A cylindrical, flat bottomed, water tight tube made of glass or metal. Its height is

approximately 115 millimeters. The inner diameter ranges from 44.2 to 45.8 millimeters.

5. Disc: Made of cork or felt, 6mm thick, with the same diameter as the inner diameter of the sleeve.

6. Gaskets: Annular, 5-6mm thick, made of cork, felt, or other appropriate materials, requiring elasticity to tightly adhere to the outer wall of the test tube, but loosely attached to the inner wall of the sleeve. At the same time, it must have sufficient hardness to maintain its shape. The purpose of the gasket is to prevent contact between the test tube and the sleeve.

7. Cold bath: metal bath cooling

8. Timer: The maximum error for measuring 30 seconds should not exceed 0.2 seconds.

Reagents and materials:


1. Sodium chloride: crystalline

2. Calcium chloride: crystalline

3. Carbon dioxide: solid

4. Cooling liquid: acetone, methanol, or naphtha

5. Wiping solution: acetone, methanol, or ethanol

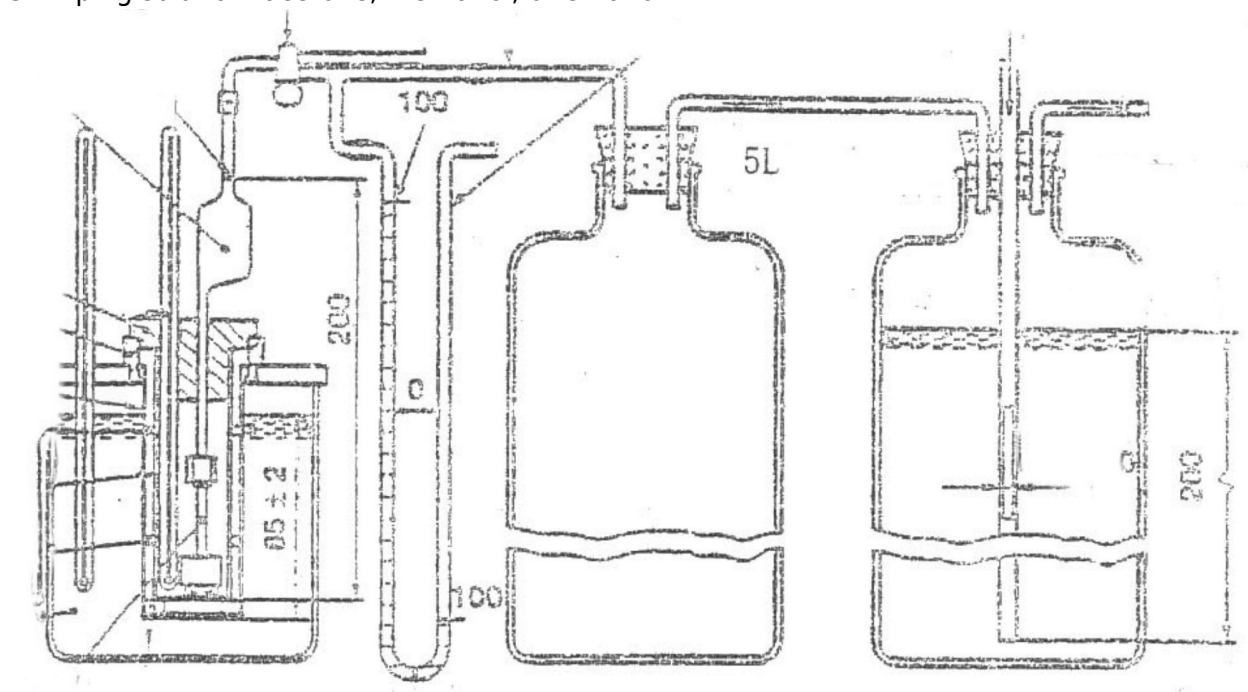

1. Test cup: made of transparent glass, flat bottomed cylindrical shape

2. Jacket: Made of brass, flat bottomed cylindrical, waterproof, can be used as an air bath.

3. Insulation ring: Made of oil resistant plastic or other suitable materials, placed at the bottom of the sleeve to provide insulation.

4. Positioning ring: Made of oil resistant plastic or other suitable materials, it surrounds the test cup and provides insulation for the test cup inside the sleeve.

5. Support ring: Made of oil resistant plastic or other suitable, non absorbent, oil resistant non-metallic materials, placed in a suitable position in a cold bath, vertically and stably suspended outside the sleeve, and the plug should be placed in the center position.

6. Plug: Made of oil resistant plastic or other suitable, non absorbent, oil resistant non-metallic materials.

7. Pipette: Made of transparent glass, there should be a marking line at a distance of $149\text{mm} \pm 0.5\text{mm}$ from the bottom of the pipette.

8. Filter: composed of brass shell, brass nut, filter screen, brass filter seat, and brass tank.
9. Three way valve: made of glass, with a bidirectional inclined hole with a diameter of 3mm.
10. Vacuum source: A vacuum pump or water pump with sufficient pressure to ensure that the air flow rate in the vacuum regulating device during the test is $15\text{L/h} \pm 1\text{L/h}$.
11. Vacuum regulating device: composed of a glass bottle, with a height of at least 350mm, capable of filling at least 5L of water and sealing it with a stopper. The stopper has three holes and is equipped with a glass tube of suitable diameter.
12. Stop watch: with an accuracy of 0.2s or higher.

Reagents and materials:

1. N-Heptane: analytically pure
2. Acetone: analytical pure
3. Lint free filter paper
4. Calibration standard

IV. Preparation

Sample preparation for cold filter plugging point

1. If there are impurities in the sample, it must be heated to above $15\text{ }^{\circ}\text{C}$ and filtered with lint free filter paper.
2. If the sample contains water, it must be dehydrated before being determined.
3. Fix the sleeve with a support ring in the hole of the cold bath cover plate, and plug the sleeve mouth tightly

4. Lower the cold bath to the following temperature:

When the cold filter plugging point of the sample is above $-3\text{ }^{\circ}\text{C}$, the cold bath temperature is $-17\text{ }^{\circ}\text{C} \pm 1\text{ }^{\circ}\text{C}$;

When the cold filter plugging point of the sample is $-4\sim-19\text{ }^{\circ}\text{C}$, the cold bath temperature is $-34\text{ }^{\circ}\text{C} \pm 1\text{ }^{\circ}\text{C}$;

When the cold filter plugging point of the sample is $-20\sim-35\text{ }^{\circ}\text{C}$, the two cold bath temperatures are $-34\text{ }^{\circ}\text{C} \pm 1\text{ }^{\circ}\text{C}$ and $-51\text{ }^{\circ}\text{C} \pm 1\text{ }^{\circ}\text{C}$.

Throughout the entire operation, the cold bath should be stirred evenly.

5. Turn on the power switch of the instrument, add liquid, and then adjust the temperature controller to the desired temperature according to the operating instructions.

6. Install the components according to the following diagram, Figure 1 (test component installation diagram) and Figure 2 (vacuum source connection diagram).

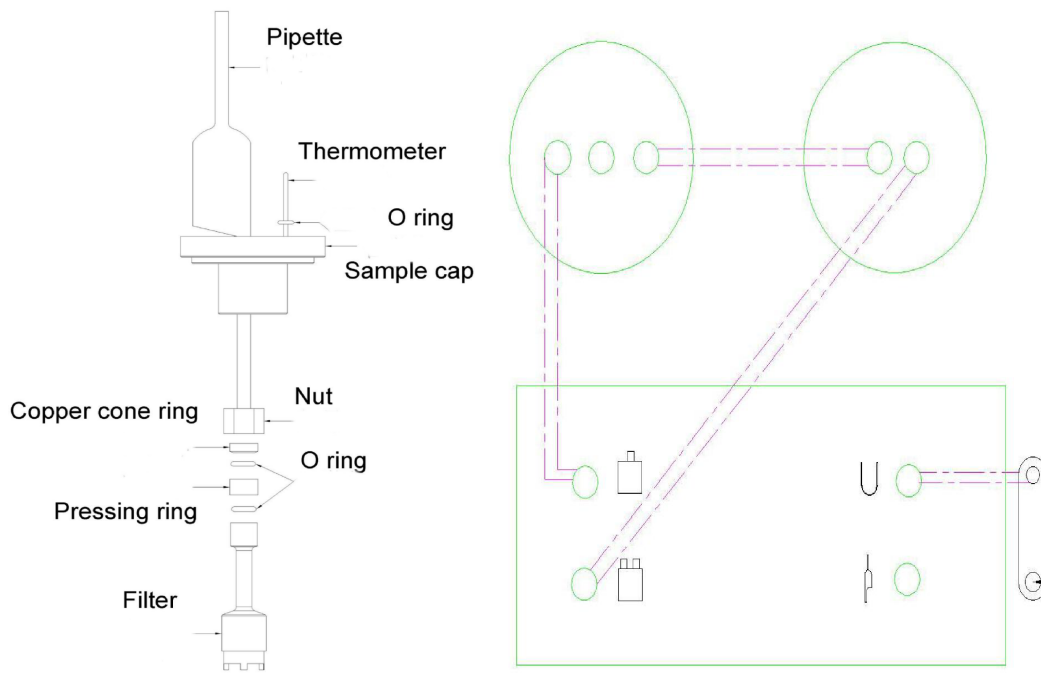


Figure 1 Figure 2

V. Operation Steps

Firstly, please carefully read the user manual to confirm the ambient temperature of the instrument ($\leq 25\text{ }^{\circ}\text{C}$). Then, use the matching connecting cable of this machine to connect the host device and connect it to the power supply. Test all device switches to check if they can display normally. If all switches are normal, immediately turn off all switches and wait for the next step of operation.

Note: The test host time cannot exceed 5 seconds at most. And the time for restarting the second time should be 10 minutes after the first time before proceeding with the operation. Please remember by the operator.

Turn on the power switch, set the temperature on the thermostat, and turn on the refrigeration switch for cold bath treatment of the sample.

Test steps for pour point

1. Pour the clean sample into the test tube until it reaches the mark. If necessary, the sample can be heated in a water bath until flowing, and then poured into a test tube. Samples that have been heated to over $45\text{ }^{\circ}\text{C}$ within 24 hours prior to the test, or samples whose heating history is unknown, must be left at room temperature for 24 hours before the test can be conducted.
2. Plug the test tube tightly with a cork with a high cloud point and high pour point thermometer inserted. If the expected pour point of the sample is higher than $36\text{ }^{\circ}\text{C}$, use a melting point thermometer. Adjust the cork to tightly plug the test tube, ensuring that the thermometer and test tube are on the same axis. Immerse the sample in the mercury bulb of the thermometer, so that the capillary starting point of the thermometer is immersed 3mm below the sample liquid level.
3. Pretreat the sample in the test tube according to point 4 or 5.
4. Samples with a pour point higher than $-33\text{ }^{\circ}\text{C}$ should be treated as follows:

4.1 Place the sample in a bath that has been maintained at 12 °C above the expected pour point, but at least 48 °C, without stirring. Heat the sample to 15 °C or 9 °C above the expected pour point (whichever is higher).

4.2 Transfer the test tube to a bath that has been maintained at 24 °C ± 1.5 °C.

When the sample reaches a temperature of 9 °C higher than the expected pour point (estimated as a multiple of 3 °C), the provisions of point 7 should be followed.

Start checking the fluidity of the sample

4.4 If the sample can still flow when the temperature has reached 27 °C, carefully remove the test tube from the bath, wipe the outer surface of the test tube with a clean cloth soaked in wiping solution, and then place the test tube in a 0 °C bath according to point 6. Observe the fluidity of the sample according to point 7 and cool it according to the procedure specified in point 8.

5. Samples with a pour point of -33 °C and below -33 °C should be treated as follows:

5.1 Heat the sample in a 48 °C bath without stirring to 45 °C, and then place it at 6 °C ± 1.5 °C. Cool to 15 °C in a bath.

When the temperature of the sample reaches 15 °C, carefully remove the test tube from the water bath and wipe the outer surface of the test tube with a clean cloth soaked in wiping solution. Then, remove the high cloud point and high pour point thermometers and replace them with low cloud point and low pour point thermometers. Place the test tubes in a 0 °C bath according to point 6, and then transfer them to each low-temperature bath according to the steps specified in point 8.

When the sample temperature reaches 9 °C higher than the expected pour point, observe the fluidity of the sample according to point 7.

6. Ensure that the inner walls of the disc, washer, and sleeve are clean and dry, and place the disc at the bottom of the sleeve. Before inserting the test tube, the disc and sleeve should be placed in a cold bath for at least 10 minutes. Place the gasket on the outer wall of the test tube, approximately 25mm from the bottom, and insert the test tube into the sleeve. Except for the 24 °C and 6 °C baths, the test tube cannot be directly placed in the cooling medium.

7. Observe the fluidity of the sample:

7.1 Starting from the first observation of temperature, the test tube should be removed from the bath or sleeve every 3 °C decrease (depending on actual usage), and the test tube should be fully tilted to determine whether the sample is flowing. The entire process of removing the test tube, observing the fluidity of the sample, and returning the test tube to the bath should not exceed 3 seconds.

7.2 From the first observation of the fluidity of the sample, the fluidity of the sample should be observed every 3 °C decrease in temperature. Special attention should be paid not to stir the lumps in the sample, nor to move the thermometer after the sample has cooled enough to form paraffin crystals. Because stirring the porous network crystals in paraffin can lead to low or incorrect results.

Note: At low temperatures, condensed water mist can hinder observation. You can use a clean cloth dipped in a wiping solution close to the temperature of the cold bath to wipe the test tube to remove the water mist on the outer surface.

7.3 When the test tube is tilted and the sample does not flow, the test tube should be immediately placed in a horizontal position for 5 seconds (measured with a timer) and the surface of the sample should be carefully observed. If the sample shows any movement, the test tube should be immediately placed back into the bath or sleeve (depending on actual usage), and the fluidity of the sample should be observed again when the temperature drops

by another 3 °C.

7.4 Continue operating in this manner until the test tube is placed in a horizontal position for 5 seconds, the sample in the test tube does not move, and the thermometer reading observed at this time is recorded.

8. If the sample is still flowing when the temperature reaches 9 °C, transfer the test tube to the next lower temperature bath and perform the same transfer at -6 °C, -24 °C, and -42 °C according to the following procedure.

- 1) The sample temperature reaches 9 °C, move to a -18 °C bath;
- 2) The sample temperature reaches -6 °C, move to -33 °C;
- 3) The sample temperature reaches -24 °C, move to a -51 °C bath;
- 4) The sample temperature reaches -42 °C, move to a bath at -69 °C.

9. For oil products whose pour point specification value is not a multiple of 3 °C, the following regulations can also be followed for determination. Start checking the fluidity of the sample when the temperature is 9 °C higher than the pour point specification value, and then observe the sample at 3 °C intervals according to the steps described in points 7 and 8 until the specification value of the sample is reached. Report whether the sample passed or did not pass the specification value.

10. For fuel oil, heavy lubricant base oil, and products containing residual fuel components, the results obtained by following the steps described in points 1-8 are the upper (highest) pour point of the sample. If it is necessary to determine the lower (lowest) pour point of the sample, it can be heated to 105 °C while stirring, and then poured into a test tube. Follow the steps described in points 2-8 to determine the lower (lowest) pour point of the sample.

11. After the above process is completed, remove the test tube from the sleeve and clean the thermometer and test tube.

Result representation

Add 3 °C to the results recorded at points 7.4 and 10 as the pour point or pour point of the sample (depending on actual usage), and take the average of the two repeated measurements as the test result.

Precision

Use the following provisions to determine the reliability of the test results (95% confidence level).

1. Repeatability

The difference between two consecutive test results obtained by the same operator, using the same instrument, and using the same method on the same sample should not exceed 3 °C.

2. Reproducibility

The difference between two test results obtained from the same sample by different operators, using different instruments, and using the same method should not exceed 6 °C.

Note: Precision was determined using 10 new (unused) mineral oil based lubricants and 16 blended fuel oils in 12 collaborative laboratories. The pour point range of mineral oil lubricating oil is -48 °C~-6 °C, and the pour point range of fuel oil is -33 °C~51 °C, resulting in the following precision.

Sample name	Repeatability	Reproducibility
Mineral oil based lubricants	2.87°C	6.43°C
Fuel oil	2.52°C	6.59°C

Test steps for cold filter plugging point

1. Install the thermometer, pipette, filter according to the schematic diagram in Figure 1, and place it in a test cup containing 45mL of sample, making the thermometer vertical. The bottom of the thermometer should be 1.3-1.7mm away from the bottom of the test cup, and the filter should also be placed vertically and exactly at the bottom of the test cup. Then, place it in a hot water bath to reach a temperature of $30\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$. Open the plug of the sleeve opening, Place the prepared test cup vertically into a copper sleeve placed in a pre cooled cold bath to a predetermined temperature. (The positioning ring should be placed inside the copper sleeve);
2. Add a water level of 100mm to U-shaped tube differential pressure gauge, and connect the silicone hoses of two 5-liter vacuum water tanks according to the schematic diagram in Figure 3,

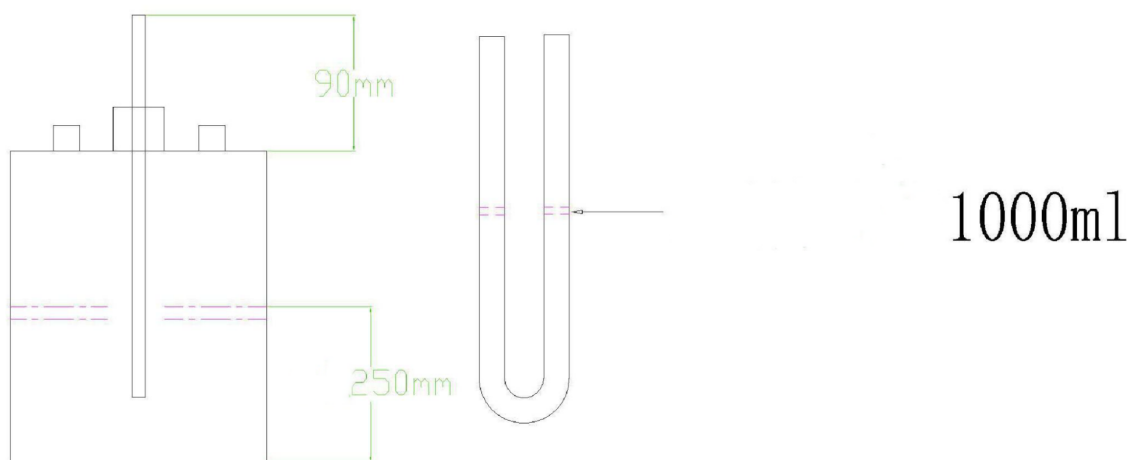


Figure 3

3. When the sample cools to 5-6 °C higher than the expected cold filter plugging point, the first measurement begins. Connect the silicone tube to the suction tube, turn on the suction switch, and at the same time, the internal stopwatch of the instrument starts timing (after the suction time reaches 1 minute, the suction will automatically stop). When the sample rises to the 20mL mark of the pipette, it indicates that the cold filter plugging point of the sample has not been reached. Turn off the suction switch to make the pipette the same as the atmosphere, and the sample naturally flows back to the test cup to continue the cooling test.
4. Repeat 2-3 steps for each 1 °C decrease until less than 20mL of sample passes through the filter within 1 minute. Record the temperature at this time, which is the cold filter plugging point of the sample. If the sample drops to -20 °C and has not yet reached its cold filter plugging point, after the sample naturally flows back to the test cup, quickly transfer the test cup to a cold bath at $-51\text{ }^{\circ}\text{C} \pm 1\text{ }^{\circ}\text{C}$ for operation until it reaches its cold filter plugging point.
5. If the expected temperature for the first measurement is lower than the cold filter plugging point of the sample, remove the test cup from the sleeve and heat it for dissolution. If the sample is abundant, it is best to pour out the cooled and melted sample, replace it with a new one, and then repeat the operation according to the previous method. If the sample is

not sufficient, it can be heated and melted to 35 °C, and then operated again according to the previous method. Heating and melting should not be repeated more than three times.

6. At the end of the experiment, remove the test cup from the sleeve, heat it to dissolve, pour out the test, and wash the test equipment. Pour 30-40mL of solvent oil into the test cup, and repeatedly suck the solvent oil four to five times from the three-way valve using an auralave. During the test, all parts of instrument wherever the sample flows through should be washed with solvent oil. Pour out the used solvent oil and repeat the washing with clean solvent oil. Finally, dry the test cup, filter, and pipette separately with a hair dryer. If there is coke or water droplets on the pipette or test cup, after washing with solvent oil once, it is also necessary to wash and blow dry with anhydrous ethanol or benzene alcohol mixed solvent. Generally, the stainless steel wire filter after 20 tests needs to be washed and replaced.

7. When the test cup is taken out of the sleeve, a plug should be inserted at the opening of the sleeve to prevent moisture in the air from condensing into water in the sleeve. During summer operation, the air humidity is high, and it is necessary to strictly prevent water condensed on the outer wall of the equipment from flowing into the sample along the pipe wall.

Precision

Use the following provisions to determine the reliability of the test results (95% confidence level).

Repeatability

The difference between two repeated measurements by the same operator should not exceed the value in equation (1).

$$r=1.2-0.027X1..... (1)$$

In the equation:

X1- The average value of two results used for comparison

Reproducibility

The difference between the two results proposed by each of the two laboratories should not exceed the value of equation (2).

$$r=3.0-0.060X2..... (2)$$

In the equation:

X2- Average value used to compare single, independent test results

VII. Common faults and troubleshooting

1. During the experiment, it is found that the host is leaking electricity. How to solve this problem?
 - a. Quickly turn off the power and check the connection points of each device and whether the insulation material of the wires is damaged.
 - b. Observe if water has been poured into the heating cabinet. If any, it should be dried before use.
2. How to deal with uneven temperature of the medium liquid during the experiment?
 - a. Check the mixing device.
 - b. Test whether the wiring of the device is in place.
 - c. After replacing the mixing device with a new one, proceed with debugging.
3. During the refrigeration process, the temperature controller always displays the temperature at the beginning of heating?
 - a. The set temperature value is lower than the temperature specified in the test.
 - b. There is a problem with the temperature sensor in the constant bath.
4. Please read the instruction manual carefully before using the instrument.
5. During the experiment, it is strictly prohibited to bring items such as lighters or matches into the laboratory to avoid a fire.
6. During the experiment, the power cord must have a good grounding terminal to ensure the safety of electricity usage.
7. When there is a malfunction in the instrument circuit, professional personnel must be consulted for maintenance.
8. When the host is not in use, the power supply and all switches should be turned off, and it should be kept in a ventilated and dry place. And all mechanical parts of the instrument should be maintained in a timely manner with lubricating oil or grease to avoid affecting their performance.
9. When discharging the medium liquid, the temperature should reach room temperature before proceeding with the operation.

VIII. Quality Assurance

The company has a one-year quality guarantee for the problems in the material or workmanship of the instrument since the date of purchase. Within the specified warranty period, if the failure of the instrument is not caused by abuse and needs to be repaired, we will carry out free maintenance. Our company will determine whether the specific failure is due to its own failure or customer abuse. For instruments beyond the warranty period, the maintenance cost will be charged as appropriate.

Exceptional case

The following conditions are not included in the warranty free maintenance:

1. Customer's own incorrect maintenance
2. Unauthorized change and abuse
3. Applying the instrument to an inappropriate environment

Package List

No.	Name	Specifications	Qty	Unit
1	Main unit	—	1	Set
2	Test tube	—	4	PC
3	Cork stopper	25*33*35mm	4	PC
4	Thermometer	-80~20℃	2	PC
5	Fuse	20 (A)	4	PC
6	Test tube pad	—	4	PC
7	Thermometer	-38~50℃	2	PC
8	Insulation board	—	1	PC
9	Hook	M3	4	PC



Biolab Scientific Ltd.

3660 Midland Avenue, Suite 300, Toronto, Ontario M1V 0B8, Canada
Email: info@biolabscientific.com | Website: www.biolabscientific.com